



CD/K/734:2010
ICS 67.120

EAST AFRICAN STANDARD

Meat and meat products — Determination of starch and glucose contents — Enzymatic method

EAST AFRICAN COMMUNITY

Foreword

Development of the East African Standards has been necessitated by the need for harmonizing requirements governing quality of products and services in East Africa. It is envisaged that through harmonized standardization, trade barriers which are encountered when goods and services are exchanged within the Community will be removed.

In order to meet the above objectives, the EAC Partner States have enacted an East African Standardization, Quality Assurance, Metrology and Test Act, 2006 (EAC SQMT Act, 2006) to make provisions for ensuring standardization, quality assurance, metrology and testing of products produced or originating in a third country and traded in the Community in order to facilitate industrial development and trade as well as helping to protect the health and safety of society and the environment in the Community.

East African Standards are formulated in accordance with the procedures established by the East African Standards Committee. The East African Standards Committee is established under the provisions of Article 4 of the EAC SQMT Act, 2006. The Committee is composed of representatives of the National Standards Bodies in Partner States, together with the representatives from the private sectors and consumer organizations. Draft East African Standards are circulated to stakeholders through the National Standards Bodies in the Partner States. The comments received are discussed and incorporated before finalization of standards, in accordance with the procedures of the Community.

Article 15(1) of the EAC SQMT Act, 2006 provides that "Within six months of the declaration of an East African Standard, the Partner States shall adopt, without deviation from the approved text of the standard, the East African Standard as a national standard and withdraw any existing national standard with similar scope and purpose".

East African Standards are subject to review, to keep pace with technological advances. Users of the East African Standards are therefore expected to ensure that they always have the latest versions of the standards they are implementing.

© East African Community 2010 — All rights reserved*

East African Community

P O Box 1096

Arusha

Tanzania

Tel: 255 27 2504253/8

Fax: 255-27-2504481/2504255

E-Mail: eac@eachq.org

Web: www.each.int

Introduction

In the preparation of this East African Standard, the following sources were consulted extensively:

ISO 13965:1998, *Meat and meat products — Determination of starch and glucose contents — Enzymatic method*

Codex Alimentarius website: http://www.codexalimentarius.net/mrls/pestdes/jsp/pest_q-e.jsp

USDA Foreign Agricultural Service website: <http://www.mrlatabase.com>

USDA Agricultural Marketing Service website: <http://www.ams.usda.gov/AMSV1.0/Standards>

USDA Plant Inspectorate Service website: http://www.aphis.usda.gov/import_export/plants

European Union: http://ec.europa.eu/sanco_pesticides/public

Assistance derived from these sources is hereby acknowledged.

Draft for comments only - Not to be cited as East African Standard

INTERNATIONAL
STANDARD

ISO
13965

First edition
1998-09-15

**Meat and meat products — Determination
of starch and glucose contents —
Enzymatic method**

*Viande et produits à base de viande — Détermination des teneurs en
amidon et en glucose — Méthode enzymatique*



Reference number
ISO 13965:1998(E)

Draft for comments only - Not to be cited as East African Standard

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 13965 was prepared by Technical Committee ISO/TC 34, *Agricultural food products*, Subcommittee SC 6, *Meat and meat products*.

Annexes A and B of this International Standard are for information only.

© ISO 1998

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland
Internet iso@iso.ch

Printed in Switzerland

Meat and meat products — Determination of starch and glucose contents — Enzymatic method

1 Scope

This International Standard specifies an enzymatic method for the determination of water-free starch content and glucose content of all kinds of meat and meat products, including poultry.

The method is suitable for the quantitative determination of starch and glucose contents down to levels of 0,30 % (*m/m*).

The method is not applicable for chemically modified starches or their derivatives.

2 Normative reference

The following standard contains provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the edition indicated was valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent edition of the standard indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*.

3 Definitions

For the purposes of this International Standard, the following definitions apply.

3.1

starch content of meat and meat products

starch content determined in accordance with the procedure described in this International Standard, and expressed as a percentage by mass

3.2


glucose content of meat and meat products

glucose content determined in accordance with the procedure described in this International Standard, and expressed as a percentage by mass

4 Principle


4.1 Hydrolysis of the starch present in a test portion with the enzyme α -amylase at pH = 5,0 for 15 min. Determination of the starch content using the following enzymatic reactions.

4.2 Hydrolysis of the solubilized starch to yield glucose using amyloglucosidase (AGS):




For the determination of the glucose content, this step is omitted.

4.3 Phosphorylation of the glucose generated by means of adenosine 5'-triphosphate (ATP) to yield glucose 6-phosphate (G-6-P) using hexokinase (HK):



4.4 Oxidation of glucose 6-phosphate (G-6-P) by means of nicotinamide adenine dinucleotide phosphate (NADP) to gluconate 6-phosphate using glucose 6-phosphate dehydrogenase (G-6-PDH):



4.5 Spectrometric measurement of the amount of reduced nicotinamide dinucleotide phosphate (NADPH) at a wavelength of 340 nm.

5 Reagents

Use only reagents of recognized analytical grade, unless otherwise specified.

5.1 Water, complying with at least grade 3 in accordance with ISO 3696.

5.2 α -Amylase (EC 3.2.1.1), enzyme suspension.

A liquid enzyme preparation of a heat-stable α -amylase produced from *Bacillus licheniformis* (Termamyl® 120L)¹.

5.3 Sodium hydroxide solution, $c(\text{NaOH}) = 5 \text{ mol/l}$.

Dissolve 200 g of sodium hydroxide in water. Cool to room temperature, dilute to 1000 ml and mix.

5.4 Sodium hydroxide solution, $c(\text{NaOH}) = 0,5 \text{ mol/l}$.

Dissolve 20 g of sodium hydroxide in water. Cool to room temperature, dilute to 1000 ml and mix.

5.5 Ammonium sulfate solution, $c[(\text{NH}_4)_2\text{SO}_4] = 3,2 \text{ mol/l}$.

Dissolve 422 g of ammonium sulfate in water. Dilute to 1000 ml and mix.

5.6 Acetate buffer, $c(\text{CH}_3\text{CO}_2\text{Na}) = 0,1 \text{ mol/l}$, pH = 5,0.

Dissolve 6,80 g of sodium acetate trihydrate ($\text{CH}_3\text{CO}_2\text{Na} \cdot 3\text{H}_2\text{O}$) in 400 ml of water. Adjust the pH to 5,0 with hydrochloric acid or sodium hydroxide solution with a pH-meter (6.2). Dilute with water to 500 ml and mix.

The solution is stable for at least 3 months at +4 °C in the dark.

5.7 Citrate buffer, $c(\text{citrate}) = 0,05 \text{ mol/l}$, pH = 4,6.

Dissolve 440 mg of citric acid monohydrate ($\text{C}_6\text{H}_8\text{O}_7 \cdot \text{H}_2\text{O}$) and 850 mg of trisodium citrate dihydrate ($\text{C}_6\text{H}_5\text{Na}_3\text{O}_7 \cdot 2\text{H}_2\text{O}$) in water. Dilute with water to 100 ml and mix. Check the pH with a pH-meter (6.2) and adjust if necessary with hydrochloric acid or sodium hydroxide solution.

The solution is stable for at least 3 months at +4 °C in the dark.

1) Termamyl® 120 L is an example of a suitable product available commercially from Novo, Denmark, and Tecator, Sweden. This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of this product.

5.8 Triethanolamine buffer, $c(\text{triethanolamine}) = 0,75 \text{ mol/l}$, $\text{pH} = 7,6$.

Dissolve 14,0 g of triethanolamine hydrochloride ($\text{C}_6\text{H}_{15}\text{NO}_3 \cdot \text{HCl}$) and 0,25 g of magnesium sulfate heptahydrate ($\text{MgSO}_4 \cdot 7\text{H}_2\text{O}$) in 80 ml of water. Set the pH at 7,6 with a pH-meter, using the sodium hydroxide solutions (5.3 and 5.4). Dilute with water to 100 ml and mix.

The solution is stable for 4 weeks at +4 °C in the dark.

5.9 Nicotinamide adenine dinucleotide phosphate solution, $c(\beta\text{-NADP-Na}_2) = 12,7 \times 10^{-3} \text{ mol/l}$.

Dissolve 100 mg of NADP disodium salt in 10,0 ml of water and mix.

The solution is stable for 4 weeks at +4 °C in the dark.

5.10 Adenosine-5'-triphosphate solution, $c(5'\text{-ATP-Na}_2\text{H}_2 \cdot 3\text{H}_2\text{O}) \approx 81 \times 10^{-3} \text{ mol/l}$.

Dissolve 500 mg of 5'-ATP- $\text{Na}_2\text{H}_2 \cdot 3\text{H}_2\text{O}$ and 500 mg of anhydrous monosodium hydrogen carbonate (NaHCO_3) in 10,0 ml of water and mix.

The solution is stable for 4 weeks at +4 °C in the dark.

5.11 Amyloglucosidase (AGS; EC 3.2.1.3), enzyme suspension in ammonium sulfate solution (5.5), $\rho(\text{AGS}) = 10 \text{ mg/ml}$.

The specific activity of the enzyme shall be 14 units per milligram.

The suspension is stable for 1 year at +4 °C in the dark.

5.12 Hexokinase (HK; EC 2.7.1.1)/glucose 6-phosphate dehydrogenase (G-6-PDH; EC 1.1.1.49), enzyme suspension in ammonium sulfate solution (5.5), $\rho(\text{HK}) = 2 \text{ mg/ml}$ and $\rho(\text{G-6-PDH}) = 1 \text{ mg/ml}$.

The specific activity of both enzymes shall be 140 units per milligram.

The suspension is stable for 1 year at +4 °C in the dark.

6 Apparatus

Usual laboratory apparatus and, in particular, the following.

6.1 Mechanical or electrical equipment, capable of homogenizing the laboratory sample.

This includes a high-speed rotational cutter, or a mincer fitted with a plate with apertures not exceeding 4,0 mm in diameter.

6.2 pH-meter.**6.3 Fluted filter papers**, glucose free, of diameter about 15 cm.

6.4 Pipettes, calibrated, for enzymatic analysis, or automatic micropipettes of equivalent quality with the following volumes: 20 μl , 50 μl , 100 μl and 200 μl .

6.5 Small plastics spatula, for mixing the contents of a cuvette (6.9).**6.6 Water bath**, capable of being maintained at $(60 \pm 2) \text{ }^\circ\text{C}$.**6.7 Hot plate.**

6.8 Spectrometer, capable of measuring at a wavelength of 340 nm.

NOTE When a spectrometer fitted with a mercury vapour lamp is available, the readings can be carried out at 365 nm and 334 nm. The molecular absorption coefficient κ for NADPH is $3,51 \text{ l}\cdot\text{mmol}^{-1}\cdot\text{cm}^{-1}$ at 365 nm and $6,18 \text{ l}\cdot\text{mmol}^{-1}\cdot\text{cm}^{-1}$ at 334 nm.

6.9 Cuvettes, made of quartz or glass, with lid, or disposable cuvettes for single use, made of polymethacrylate, of 10 mm optical path length.

6.10 Analytical balance, capable of weighing to the nearest 0,1 mg.

7 Sampling

Sampling is not part of the method specified in this International Standard. A recommended sampling method is given in ISO 3100-1 [1].

It is important that the laboratory receive a sample which is truly representative and has not been damaged or changed during transport or storage.

Start from a representative sample of at least 200 g. Store the sample in such a way that deterioration and change in composition are prevented.

8 Preparation of test sample

Homogenize the laboratory sample with the appropriate equipment (6.1). Take care that the temperature of the sample material does not rise above 25 °C. If a mincer is used, pass the sample at least twice through the equipment.

Fill a suitable airtight container with the prepared sample. Close the container and store in such a way that deterioration and change in composition are prevented. Analyse the sample as soon as practicable, but always within 24 h after homogenization.

9 Procedure

NOTE Muscle glycogen, which occurs normally in, for example, sausages, does not interfere with the determination. Maltose interferes because this disaccharide is hydrolysed by amyloglucosidase into glucose. Maltose (and glucose) can, however, be extracted from the sample with alcohol.

9.1 Test portion

If the test sample contains maltose, make sure that the water content does not exceed 20 % (m/m). If necessary, dry the test sample.

Weigh about 400 mg of the prepared test sample (see clause 8) to the nearest 0,1 mg into a centrifuge tube. Proceed in accordance with 9.2.

If the test sample does not contain maltose, weigh between 100 mg and 1,0 g (m) of the prepared test sample to the nearest 0,1 mg into a 100 ml conical flask.

Add 30 ml of acetate buffer (5.6) and proceed in accordance with 9.3.

9.2 Extraction of maltose (and glucose)

Wash the sample three times with 10 ml of 40 % (V/V) ethanol and centrifuge after each washing. Filter the supernatant. Combine the precipitate in the centrifuge tube with that on the filter and transfer to a 100 ml conical flask using 4 x 5 ml of acetate buffer (5.6). Add 10 ml of acetate buffer (5.6).

9.3 Preparation of extract

Pipette (6.4) 50 μl of α -amylase suspension (5.2) into the conical flask containing the sample. Cover the conical flask with aluminium foil and boil on a hot plate (6.7) for 15 min. Shake the flask at intervals.

Then keep the conical flask at 60 °C in the water bath (6.6) for 15 min. Quantitatively transfer the contents of the conical flask to a 100 ml volumetric flask. Rinse the conical flask with warm water and add the washings to the volumetric flask. Allow to cool to room temperature and dilute to the mark with water. Filter (6.3) at least 10 ml of the sample extract, discarding the first few millilitres, and immediately proceed in accordance with 9.4.

Keep samples containing fat for 1 h in the refrigerator before filtration.

9.4 Determination

9.4.1 Prepare a reagent blank solution as follows. Pipette (6.4) 200 μl of citrate buffer (5.7) and 100 μl of water into a cuvette (6.9) containing a spatula (6.5).

9.4.2 Prepare a test solution for the glucose determination as follows. Pipette (6.4) 200 μl of citrate buffer (5.7) and 100 μl (V_2) of the sample extract (9.3) into a cuvette (6.9) containing a spatula (6.5).

9.4.3 Prepare a test solution for the starch determination as follows. Pipette (6.4) 200 μl of citrate buffer (5.7) and 100 μl (V_2) of the sample extract (9.3) into a cuvette (6.9) containing a spatula (6.5).

If the concentration of starch in the sample solution exceeds 0,4 g/l, dilute it before analysis.

9.4.4 Pipette (6.4) 20 μl of AGS suspension (5.11) into the cuvette containing the reagent blank solution (9.4.1) and into the cuvette containing the test solution for the starch determination (9.4.3). Pipette 20 μl of water into the cuvette containing the test solution for the glucose determination (9.4.2).

Mix the contents of the cuvettes by swirling or by moving the spatula up and down.

Close the cuvettes with the lid or otherwise (e.g. paraffin sheet). Keep the cuvettes in the water bath (6.6) for 15 min at (60 ± 2) °C.

The above pipette procedure is schematically presented below:

Reagent	Reagent blank solution	Test solution for glucose determination	Test solution for starch determination
Citrate buffer (5.7)	200 μl	200 μl	200 μl
Sample extract (9.3)	—	100 μl	100 μl
Water (5.1)	100 μl	20 μl	—
AGS suspension (5.11)	20 μl	—	20 μl

The volume of sample extract pipetted into the cuvette may be increased up to 1,0 ml of aqueous solution. In this case, adjust the pH of the filtrate to pH = 4 to pH = 5. Accordingly reduce the volume of 1,50 ml of water to be added to the reaction mixture in 9.4.5, in order to obtain the same final volume V_1 in 9.4.6.

9.4.5 Cool the cuvettes to $(22,5 \pm 2,5)$ °C and clean their outside surfaces. Pipette (6.4) successively to all cuvettes 1,00 ml of the triethanolamine buffer (5.8), 100 μl of the NADP solution (5.9), 100 μl of the ATP solution (5.10) and 1,50 ml of water. Mix carefully by swirling or with the spatula (6.5).

Read the absorbance A_1 (6.8) of each cuvette at a wavelength of 340 nm against water after 3 min.

9.4.6 Pipette (6.4) into each of the cuvettes 20 μl of HK/G-6-PDH suspension (5.12). Mix the contents of the cuvettes by moving the spatula up and down. The final cuvette volume is 3,04 ml (V_1).

Read the absorbance A_2 of each cuvette at a wavelength of 340 nm against water after 15 min.

NOTE The reaction is normally completed within 5 min to 10 min. If the reaction does not stop within this time, repeat this reading every 2 min until a constant increase of absorbance every 2 min is detected. Extrapolate the absorbance to the time of addition of the enzyme HK/G-6-PDH (for an example, see figure A.1).

10 Calculation

10.1 Water-free starch content

10.1.1 Absorbance difference

Calculate the absorbance difference using the equation

$$\Delta A_s = (A_{2s} - A_{1s}) - (A_{2g} - A_{1g}) - (A_{2b} - A_{1b})$$

where

- ΔA_s is the absorbance difference due to the starch content;
- A_{1b} is the absorbance measured in 9.4.5 of the reagent blank solution;
- A_{1g} is the absorbance measured in 9.4.5 of the test solution for the glucose determination;
- A_{1s} is the absorbance measured in 9.4.5 of the test solution for the starch determination;
- A_{2b} is the absorbance measured in 9.4.6 of the reagent blank solution;
- A_{2g} is the absorbance measured in 9.4.6 of the test solution for the glucose determination;
- A_{2s} is the absorbance measured in 9.4.6 of the test solution for the starch determination.

10.1.2 Calculation of water-free starch content

Calculate the water-free starch content using the equation

$$w_s = \frac{\Delta A_s \times M_{rgs} \times V_1 \times f \times 100}{d \times \kappa \times m \times V_2 \times 1000 \times 10}$$

where

- w_s is the numerical value of the water-free starch content, as a percentage by mass, of the test sample;
- ΔA_s is the absorbance difference calculated in 10.1.1;
- M_{rgs} is the relative molecular mass of glucose in starch ($M_{rgs} = M_{rglucose} - M_{rwater} = 162,1$);
- V_1 is the numerical value of the final volume, in millilitres, in the cuvette ($V_1 = 3,04$ ml);
- f is the dilution factor;
- d is the numerical value of the optical path length, in centimetres, of the cuvette;
- κ is the numerical value of the molar absorption coefficient, in litres per millimole centimetre, of NADPH ($\kappa = 6,30$ when measured at 340 nm);
- m is the numerical value of the mass, in grams, of the test portion (9.1);
- V_2 is the numerical value of the volume, in millilitres, of sample extract added in 9.4.3.

Round the result to two decimal places.

10.2 Glucose content

10.2.1 Absorbance difference

Calculate the absorbance difference using the equation

$$\Delta A_g = (A_{2g} - A_{1g}) - (A_{2b} - A_{1b})$$

where

ΔA_g is the absorbance difference due to the glucose content;

A_{1b} is the absorbance measured in 9.4.5 of the reagent blank solution;

A_{1g} is the absorbance measured in 9.4.5 of the test solution for the glucose determination;

A_{2b} is the absorbance measured in 9.4.6 of the reagent blank solution;

A_{2g} is the absorbance measured in 9.4.6 of the test solution for the glucose determination.

10.2.2 Calculation of glucose content

Calculate the glucose content using the equation

$$w_g = \frac{\Delta A_g \times M_{rg} \times V_1 \times f \times 100}{d \times \kappa \times m \times V_2 \times 1000 \times 10}$$

where

w_g is the numerical value of the glucose content, as a percentage by mass, of the test sample;

ΔA_g is the absorbance difference calculated in 10.2.1;

M_{rg} is the relative molecular mass of glucose ($M_{rg} = 180,2$);

V_1 is the numerical value of the final volume, in millilitres, in the cuvette ($V_1 = 3,04$ ml);

f is the dilution factor;

d is the numerical value of the optical path length, in centimetres, of the cuvette;

κ is the numerical value of the molar absorption coefficient, in litres per millimole centimetre, of NADPH ($\kappa = 6,30$ when measured at 340 nm);

m is the numerical value of the mass, in grams, of the test portion (9.1);

V_2 is the numerical value of the volume, in millilitres, of sample extract added in 9.4.2.

Round the result to two decimal places.

11 Precision

11.1 Repeatability

11.1.1 Water-free starch content

The absolute difference between two independent single test results, obtained using the same method on identical test material with starch contents between 0,3 % (m/m) and 4,0 % (m/m) in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases exceed the repeatability limit r_s given by the equation:

$$r_s = 0,102 + 0,132 \times \bar{w}_s$$

where

r_s is the numerical value of the repeatability limit, as a percentage by mass, for water-free starch content;

\bar{w}_s is the mean of the two results for water-free starch content.

11.1.2 Glucose content

The absolute difference between two independent single test results, obtained using the same method on identical test material with glucose contents between 0,3 % (*m/m*) and 1,2 % (*m/m*) in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases exceed the repeatability limit r_g given by the equation:

$$r_g = 0,197 + 0,070 \times \bar{w}_g$$

where

- r_g is the numerical value of the repeatability limit, as a percentage by mass, for glucose content;
- \bar{w}_g is the mean of the two results for glucose content.

11.2 Reproducibility

11.2.1 Water-free starch content

The absolute difference between two single test results obtained using the same method on identical test material with starch contents between 0,3 % (*m/m*) and 5,0 % (*m/m*) in different laboratories with different operators using different equipment, will in not more than 5 % of cases exceed the reproducibility limit R_s given by the equation:

$$R_s = 0,229 + 0,232 \bar{w}_s$$

where

- R_s is the numerical value of the reproducibility limit, as a percentage by mass, for water-free starch content;
- \bar{w}_s is the mean of the two results for water-free starch content.

11.2.2 Glucose content

The absolute difference between two single test results obtained using the same method on identical test material with glucose contents between 0,3 % (*m/m*) and 1,2 % (*m/m*) in different laboratories with different operators using different equipment, will in not more than 5 % of cases exceed the reproducibility limit R_g given by the equation:

$$R_g = 0,232 + 0,086 \times \bar{w}_g$$

where

- R_g is the numerical value of the reproducibility limit, as a percentage by mass, for glucose content;
- \bar{w}_g is the mean of the two results for glucose content.

12 Test report

The test report shall specify:

- all information necessary for the complete identification of the sample;
- the sampling method used, if known;
- the test method used, with reference to this International Standard;
- all operating details not specified in this International Standard, or regarded as optional, together with details of any incidents which may have influenced the test result(s);
- the test result obtained; or
- if the repeatability has been checked, the final quoted result obtained.

Annex A (informative)

Example of plotting and extrapolation of absorbance values

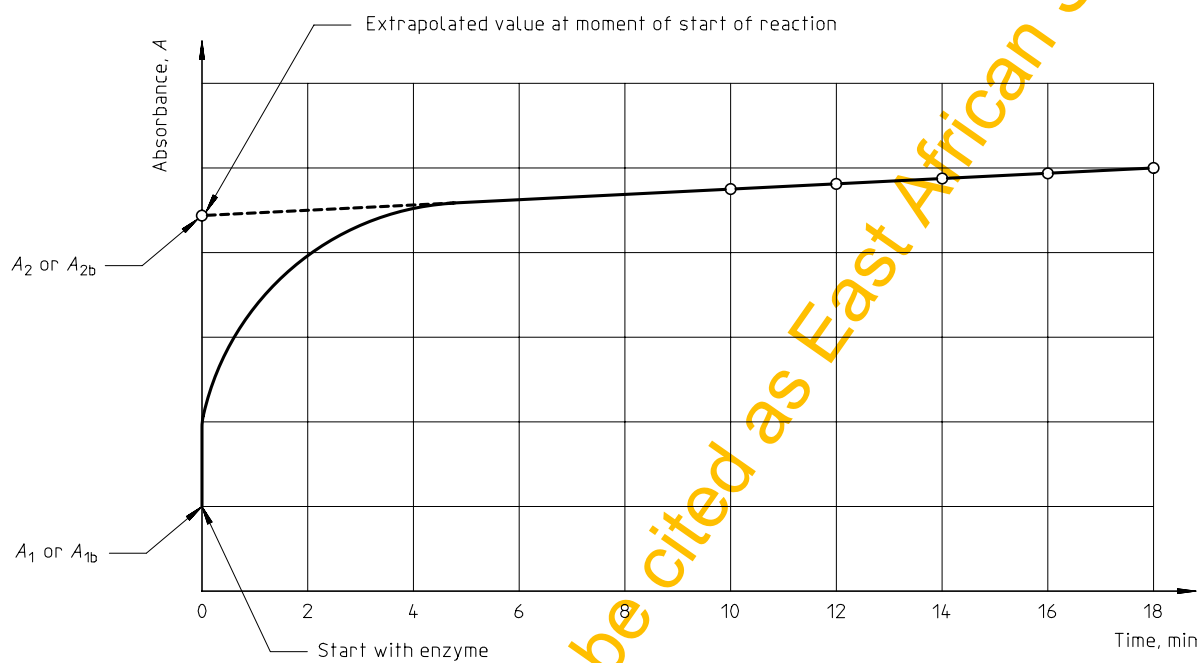


Figure A.1 — Example of plotting and extrapolation of absorbance values

Annex B (informative)

Bibliography

- [1] ISO 3100-1:1991, *Meat and meat products — Sampling and preparation of test samples — Part 1: Sampling*.
- [2] ISO 5725-1:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 1: General principles and definitions*.
- [3] ISO 5725-2:1994, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*.
- [4] Method No. 145 (1993). *Starch and Glucose: Enzymatic Determination in Foods*. Nordic Committee on Food Analysis (NMKL), Esbo, Finland (in English and Scandinavian) (UDC 577.1-5.08:641.13).
- [5] Method No. 07.00-25 (1983). *Determination of Starch in Meat Products*. Amtliche Sammlung von Untersuchungsverfahren nach Paragraph 35 LMBG (in German).

Draft for comments only - Not to be cited as East African Standard

Draft for comments only - Not to be cited as East African Standard

ICS 67.120.10

Descriptors: agricultural products, food products, animal products, meat, meat products, chemical analysis, determination of content, starches, glucose, enzymatic methods.

Price based on 10 pages

Draft for comments only - Not to be cited as East African Standard